

Standard Operating Procedure for the
Analysis of Fresh Water Samples for
Orthophosphorus
CCAL 34B.2

Cooperative Chemical Analytical Laboratory
College of Forestry
Oregon State University
321 Richardson Hall
Corvallis, Oregon

Prepared by Kathryn Motter
And Cameron Jones
Revised April 2014

**Standard Operating Procedure for the
Analysis of Fresh Water Samples for Orthophosphorus
CCAL 34B.2**

Table of Contents

1.0	Scope and Application	3
2.0	Summary of Method	3
3.0	Definitions	3
4.0	Interferences	4
5.0	Safety	4
6.0	Equipment and Supplies.....	4
7.0	Reagents and Standards	5
7.1	Preparation of Reagents	5
7.2	Preparation of Standards	6
8.0	Sample Handling and Storage.....	7
9.0	Quality Control	7
10.0	Calibration and Standardization	7
11.0	Procedure	8
11.1	Calibration and Analysis Procedure.....	8
11.2	System Notes.....	8
12.0	Data Analysis and Calculations	8
13.0	Method Performance	9
14.0	Pollution Prevention	9
15.0	Waste Management.....	9
16.0	References	10
17.0	Tables, Diagrams, Flowcharts, and Validation Data.....	10
17.1	Orthophosphorus Reaction Manifold.....	11
17.2	Orthophosphorus Manifold Specifications	11
17.3	Data System Parameters	11
18.0	Document Revision History.....	12

Standard Operating Procedure for the Analysis of Fresh Water Samples for Orthophosphorus CCAL 34B.2

1.0 Scope and Application

- 1.1 This method covers the determination of orthophosphorus in fresh waters in the range of 0.001 - 0.200 mg P/L. Sample concentrations greater than 0.200 mg P/L can be analyzed by dilution of the sample prior to analysis, or calibration to a higher range.

2.0 Summary of Method

- 2.1 Phosphorus occurs in fresh waters almost solely in the form of various phosphates. Phosphates that can be analyzed colorimetrically without preliminary acid hydrolysis or oxidative digestion are defined as “reactive phosphorus”. Soluble reactive phosphorus (SRP) exists in both dissolved and suspended forms. It is predominately composed of orthophosphorus, but may include a small fraction of condensed phosphate inevitably hydrolyzed during the procedure. Because of this predominance of orthophosphorus, reactive phosphorus is commonly called orthophosphorus, as it is within this method. Orthophosphorus is determined colorimetrically by reaction of ammonium molybdate and antimony potassium tartrate to form phosphomolybdic acid, which is then reduced to intensely colored molybdenum blue by ascorbic acid.

3.0 Definitions

- 3.1 DI water: Water that has been through a deionization system to produce water similar to ASTM Type I reagent with 16.7 Mohms resistivity (ASTM) (Reference 16.3).
- 3.2 Method Detection Limit (MDL): The minimum concentration of an analyte that can be measured and reported with 99% confidence, based on a one-sided 99% confidence interval (t -value at a significance level of 0.01 and $n-1$ degrees of freedom) from at least seven repeated measurements of a low concentration standard measured within an analysis run.

$$\text{MDL} = ts$$

Where,

t = Student's t value at a significance level of 0.01 and $n-1$ degrees of freedom

s = standard deviation of at least seven repeated measurements of a low level standard

4.0 Interferences

- 4.1 Arsenates at concentrations as low as 0.1 mg/l, react with molybdate reagent to produce a blue color resulting in positive interference in colorimetric analysis at 880 nm.
- 4.2 Nitrite and hexavalent chromium interfere to give low analytical results at concentrations as low as 1.0 mg/l.

5.0 Safety

- 5.1 The toxicity or carcinogenicity of each reagent has not been precisely determined; however, each chemical should be regarded as a potential health hazard. Exposure to these chemicals should be reduced to the lowest possible level. Cautions are included for known extremely hazardous materials.
- 5.2 The following chemicals have the potential to be highly toxic or hazardous. For detailed explanations, consult the MSDS.
 - 5.2.1 Sulfuric acid
 - 5.2.2 Antimony potassium tartrate
 - 5.2.4 Potassium persulfate

6.0 Equipment and Supplies

Note: *Brand names, suppliers and part numbers are for illustrative purposes only. No endorsement is implied. Equivalent performance may be achieved using apparatus and materials other than those specified here, but demonstration of equivalent performance that meets the requirements of this method is the responsibility of the laboratory.*

- 6.1 Balance measuring to at least 0.1 mg
- 6.2 Volumetric flasks and pipettes as required

- 6.3 Technicon Auto-Analyzer II
 - 6.3.1 Multichannel proportioning pump
 - 6.3.2 Colorimetric Detector
 - 6.3.3 Data system
 - 6.3.4 Alpkem manifold and method 155-71W/modified
- 6.4 Safety glasses
- 6.5 Nitrile gloves
- 6.6 Lab coat or apron
- 6.7 Laboratory Exhaust Fume Hood
- 6.8 High density polyethylene (HDPE) bottles

7.0 Reagents and Standards

7.1 Preparation of Reagents

Solution 7.1.3 and 7.1.7 need to be filtered through a prewashed GF/F filter after preparation

- 7.1.1 *Sulfuric acid solution, 5 N*

Slowly add 140 ml of concentrated H₂SO₄ to 700 mL of DI water over an ice bath. Equilibrate to room temperature and bring up to 1000 mL with DI water.
- 7.1.2 *Antimony potassium tartrate solution*

Dissolve 1.3715 g antimony potassium tartrate (C₈H₄K₂Sb₂O₁₂ · 3 H₂O) in 400 mL DI water in a 500 ml volumetric flask. Bring to volume with DI water. Store at room temperature. Stable at least six months.
- 7.1.3 *Ammonium molybdate solution*

Add 20 g (NH₄)₆Mo₇O₂₄ · 4H₂O to a 500 mL volumetric flask and fill to the mark with DI water. Swirl until dissolution complete. Store in a brown glass bottle in the dark at room temperature. Good until precipitate forms, but no longer than one month.
- 7.1.4 *Ascorbic acid, 0.1 M*

Transfer 1.8 g of ascorbic acid to a 100 mL volumetric flask and dilute to the mark with DI water. The solution is stable for two days if stored refrigerated. Bring to room temperature before use.
- 7.1.5 *Combined color reagent*

To prepare 200 mL of color reagent, mix reagents in the following proportions and in the order given. All reagents must be at room temperature before they are mixed. The reagent will be clear with a yellow-green tint. Total volume may be adjusted proportionately.

100 ml	5N H ₂ SO ₄
10 ml	Antimony potassium tartrate solution
30 ml	Ammonium molybdate solution
60 ml	Ascorbic acid

The reagent must be prepared fresh daily. Make only as much reagent as will be needed for that days analyses. Discard solution if the color deteriorates (i.e., gets darker or precipitates). The reagent must be stored in the dark.

7.1.6 *SLS Water*

Dissolve 0.353 g of sodium lauryl sulfate in 2.0 mL of DI water. Add this solution to 200 mL of DI water.

7.1.7 *EDTA Reagent*

Place 6 pellets of NaOH in approximately 500 mL of DI water and dissolve completely. Add 50 g disodium ethylenediamine tetraacetate dihydrate. Dissolve completely and dilute to 1 L. Filter. Reagent is stable.

7.2 Preparation of Standards

7.2.1 *Calibration Standards:*

Standards are prepared by dilution of a standard purchased from a vendor that provides traceability to NIST standards. A mixed stock standard is prepared by dilution of the purchased reagent to an intermediate concentration. The stock standard with various concentrations of each ammonia, nitrate, and phosphorus is used to prepare working standards in the table below.

	mg NH ₃ -N/L	mg NO ₃ -N/L	mg PO ₄ P/L
1	0.010	0.005	0.010
2	0.050	0.025	0.050
3	0.100	0.050	0.100
4	0.200	0.100	0.200

7.2.2 *Second Source Check Standard:*

Standards are prepared by dilution of a standard purchased from a vendor that provides traceability to NIST standards; this reagent is from a source other than that of the calibration standards. A mixed stock standard is prepared by dilution of the purchased reagent to an intermediate concentration. Check standard concentrations are the same as calibration standard 3.

8.0 Sample Handling and Storage

- 8.1 If required, unfiltered samples are filtered upon receipt through glass fiber filters into clean HDPE bottles and stored at 4°C in the dark. Samples should be analyzed within 48 hours to ensure sample integrity. If samples must be held prior to analysis, they are stored frozen at -18°C.

9.0 Quality Control

- 9.1 Preparation of stock standards is recorded on worksheets and documented by weight of standard added to a given flask before dilution to volume with DI water. All records of certification are kept on file at CCAL Laboratory.
- 9.2 Blank: DI water run before the calibration.
- 9.3 Method Detection Limit (MDL): Established for each analyte. Based on a one-sided 99% confidence interval (t-value) from at least seven repeated measurements of a low concentration standard. The t-distribution value is multiplied by the standard deviation of the population (n-1) to obtain the MDL.
- 9.4 Analytical Duplicate: Separate analysis from the same sample aliquot. Run a minimum of once every analysis set.
- 9.5 Standard recoveries are tracked over time to monitor overall performance.

10.0 Calibration and Standardization

- 10.1 Balances: calibrated yearly by external vendor.
- 10.2 Pipette delivery checked by weight to within 2% of theoretical weight of aliquot volume.
- 10.3 Calibration curve with $r^2 \geq 0.995$. (See 17.3 for calibration data set-up.)
- 10.4 Calibration verification with check standards, monitored throughout the run. If measurement exceeds +/- 10% of the theoretical value, the analysis should be terminated and the instrument recalibrated. The calibration must be verified before continuing analysis.

11.0 Procedure

11.1 Calibration and Analysis Procedure

- 11.1.1 Prepare reagents and standards as outlined in Section 7.
- 11.1.2 Set up manifolds as shown in Section 17.1.
- 11.1.3 Samples are injected into the reaction path at a fixed time interval, determined by the cam timing set in the auto-sampler. Setup or confirm data system parameters as detailed in Section 17.3.
- 11.1.4 Pump DI water through all reagent and sample lines. Check for leaks and stable bubble pattern (smooth flow). Pump reagents through all lines until the system equilibrates (minimum of one hour).
- 11.1.5 Record sample id's in the data template.
- 11.1.6 Calibrate the instrument with standards. Calibration regression equations must have $r^2 \geq 0.995$.

11.2 System Notes

- 11.2.1 If the baseline is excessively noisy, clean the manifold using the following procedure:
 - Place all reagent and carrier lines in rinse water and pump to clear reagents.
 - Place all lines in alkaline EDTA for several minutes.
 - Place lines in DI water and pump until thoroughly rinsed.
- 11.2.2 If baseline has a large number of air spikes, check pump tubes for excessive wear and replace as necessary.
- 11.2.3 Poor sensitivity or insufficient color development may be the result of old ammonium molybdate solution. Prepare fresh and flush system thoroughly.
- 11.2.4 Turbidity and color that persists in the sample after filtration may absorb at the 880 nm. Reanalyze samples with color reagent prepared without ascorbic acid as turbidity/color blanks. Any response from the turbidity/color blanks must then be subtracted from the initial analysis response.

12.0 Data Analysis and Calculations

- 12.1 The data system prepares a calibration curve by plotting response of injected standards versus known standard concentration. The resulting regression equation is used to calculate the sample concentration.

- 12.2 All results and sample information are filed in the analysis data system by analysis run. Details specific to the instrumental analysis are noted in the Instrument Run Log created and maintained for the AAIL. Analytical results are entered into electronic format and entries are verified by a second person.

13.0 Method Performance

- 13.1 This method was validated through inter-laboratory studies. The CCAL Water Analysis Laboratory participates in the USGS Standard Reference Water QA program and the National Water Research Institute's (NWRI) Environment Canada Proficiency Testing (PT) Program.

14.0 Pollution Prevention

- 14.1 The chemicals used in this method pose little threat to the environment when properly managed.
- 14.2 All standards and reagents should be prepared in volumes consistent with laboratory use to minimize the volume of disposable waste.
- 14.3 For further information on pollution prevention consult *Less is better: Laboratory Chemical Management for Waste Reduction*, available from the American Chemical Society's Department of Government Relations and Science Policy, 1155 16th Street NW, Washington D.C. 20036, (202) 872-4477.

15.0 Waste Management


- 15.1 It is the laboratory's responsibility to comply with all federal, state and local regulations governing waste management, and to protect the environment by minimizing and controlling all releases from fume hoods and bench operations. Compliance with all sewage discharge permits and regulations is required.
- 15.2 For further information on waste management, consult "The Waste Management Manual for Laboratory Personnel", and "Less is Better: Laboratory Chemical Management for Waste Reduction", both available from the American Chemical Society's Department of Government Relations and Science Policy, 1155 16th Street NW, Washington DC, 20036.

16.0 References

- 16.1 Standard Methods For The Examination of Water and Wastewater, Method 4500-P Phosphorus; 4500-P F. Automated Ascorbic Acid Reduction Method. American Public Health Association. 21st Edition, 2005.
- 16.2 Code of Federal Regulations. Protection of Environment. Section 40, Appendix B to Part 136. Definition and procedure for the determination of the method detection limit. Revision 1.11. Revised July 1, 1990. Office of the Federal Register, National Archives and Records.
- 16.3 ASTM. American Society for Testing and Materials. Standard Specifications for Reagent Water. D1193-77 (Reapproved 1983). Annual Book of ASTM Standards, Vol. 11.01. ASTM: Philadelphia, PA, 1991.
- 16.4 FWPCA Methods for Chemical Analysis of Water and Wastes.
- 16.5 Murphy J., and J. Riley. "A Modified Single Solution Method for the Determination of Phosphate in Natural Waters." *Anal. Chem. Acta.* 27, 31. 1962.
- 16.6 Gales, M. E., Jr., E. C. Julian, and R. C. Kroner. "Method for Quantitative Determination of Total Phosphorus in Water." *J. AWWA* 58:1363. 1966.
- 16.7 American Water Works Assoc. 1958. Committee Report. "Determination of Ortho Phosphate, Hydrolyzable Phosphate and Total Phosphate in Surface Waters." *J. Am. Water Works Assoc.* 50:1563.
- 16.8 Strickland, J. D. H. and T. R. Parsons. 1965. *A Manual of Sea Water Analysis*, 2nd Ed. Fish Res. Bd., Ottawa, Canada.

17.0 Tables, Diagrams, Flowcharts, and Validation Data

17.1 Orthophosphorus Reaction Manifold

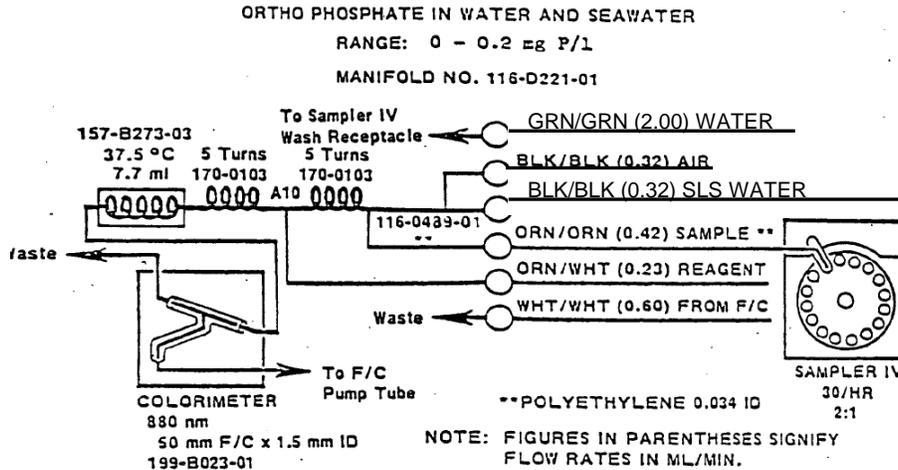

17.2 Orthophosphorus Manifold Specifications

Carrier is SLS water reagent

Interference filter is 880 nm

Pump tubing is Tygon

Manifold tubing is 0.030 mm i.d.

Mixing coils are 5 turn with an injection “T” fitting between coils.

15 mm x 2 mm flow cell

17.3 Data System Parameters

Cycle throughput: 30 samples/hr

Cycle Period: 120 s

Analyte Data:

Concentration Units mg PO₄-P/L

Calibration Data:

Level	1	2	3	4
Concentration mg/L	0.010	0.050	0.100	0.200

Calibration Fit Type: linear regression

Sampler Timing:
Minimum Probe in Wash Period: 30 s
Probe in Sample Period: 90 s

18.0 Document Revision History

Original Document: April 2006

Version: 40A.0

Title: Standard Operating Procedure for the Analysis of Fresh Water Samples for Orthophosphorus

Edit Date: July 2008

New Version: 34B.0

Document updated to reflect change to automated method of analysis

Edit Date: February 2010

New Version: 34B.1

Address update

Section 7.2: delete silica from mixed standard

Section 13.1: add Environment Canada Proficiency Testing Program participation.

Edit Date: April 2014

New Version: 34B.2

Section 1: change working range of method for appropriate significant figures.

Section 7.1: update reagent preparation of sodium laurel sulfate. Add EDTA cleaning reagent preparation.

Section 8.0: add specific sample hold time.

Section 11.2: change cleaning reagent.

Section 17.2: change carrier.

General editing.